

Are zirconias of today different?



Background

The advantages of ceramic materials are generally considered to be their tooth-like translucent appearance, their good biological compatibility in direct contact with the gingiva and a wear pattern that is comparable to that of enamel. These criteria are usually met by lithium silicate ceramics, which are indicated for veneers, tabletops, single crowns and small anterior bridges. If we wish to expand the indication range and integrate larger restorations in the posterior region, this objective is only achievable with zirconia ceramics [7]. However, the higher fracture strength

of zirconia is obtained at the expense of an opaque, less tooth-like appearance. This fact was initially not disturbing because the opaque framework was veneered with feldspathic ceramics. Since it has become technically possible, using the CAD/CAM process, to produce not only frameworks made of zirconia, but also complete restorations with occlusal surfaces, the high opacity of zirconia is no longer desirable from a clinical point of view. Developments in recent years have aimed to develop zirconias with the above-mentioned properties of silicate ceramics, which include combining translucency, bio-

compatibility, a tooth-like wear pattern with higher fracture strength and the possibility of CAD/CAM processing. These efforts have resulted in the development of different types of zirconia.

The crystal structure of zirconium dioxide (Fig. 1, Fig. 2) can be influenced by doping it with different amounts of yttrium and/or aluminum [13]. Zirconia exists in varying phases which depend on temperature; these are the cubic (> 2370°C), tetragonal (> 1170°C) or monoclinic (room temperature) phases; moreover, phase transitions are accompanied by a change in volume. In the case of opaque “conventional zirconia”, for example, tetragonal fractions can be stabilized at room temperature by doping them with 3 mol% yttrium oxide (3Y-TZP, 3 mol% yttria stabilized tetragonal zirconia polycrystal). This allows a spontaneous phase transformation to take place within the monoclinic crystal structure in response to mechanical stress. The increase in volume that occurs can, for instance, counteract the propagation of cracks.

Today we distinguish several generations or classes of zirconia [13]:

- 1st Generation 3Y-TZP-A → flexural strength > 1000 MPa → opaque
- 2nd Generation 3Y-TZP-LA → flexural strength 900 MPa 5 % → more translucent
- 3rd Generation 5Y-TZP → flexural strength 600 MPa 15 % → more translucent
- 4th Generation 4Y-TZP → flexural strength 750 MPa 10 % → more translucent

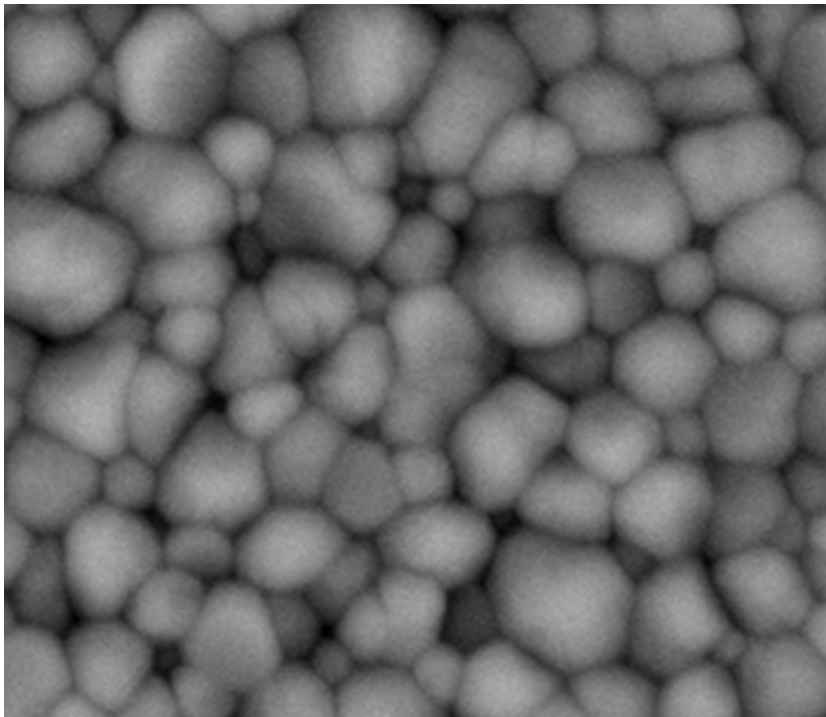


Figure 1 Scanning electron microscope imaging of the surface of 3Y-zirconia (magnification: 10,000x)

Translation from German: Cristian Miron

Citation: Behr M, Füllerer J, Strasser T, Preis V, Zacher J: Are zirconias of today different? Dtsch Zahnärztl Z Int 2020; 2: 114–118

DOI.org/10.3238/dzz-int.2020.0114-0118

- 5th Generation 3Y/4Y/5Y-TZP → flexural strength 550–1200 MPa 1–15 % → more translucent (Multilayer with translucency gradients)

In a first step to make 3Y-TZP more translucent, the aluminum content was reduced in the 2nd generation. Yet, only the 3rd and 4th generations of zirconia show considerably improved translucency. However, they achieve higher translucency at the expense of lower strength, with values being similar to those of lithium disilicate ceramics. The newest development in zirconias are “Multilayer”; they combine areas of “highly” translucent and opaque zirconium dioxide in several layers within the same milling block (Fig. 3). By skillfully aligning the digitally planned restoration in the milling block for the milling machine, larger bridges in the posterior region can also be fabricated with a more natural color gradient. However, it is important to note that the more translucent areas of the milling blocks have a lower strength than the opaquer areas. This can result in clinical failures if the mixed blank is incorrectly planned and set up in the milling machine, as though the same flexural strengths were present in all areas of the blank. Furthermore, initial investigations on the strength of various Multilayer zirconias showed that the strength in the transition layer (interphase) could be a weak point [5]. The strength of this “transition layer” was about 30 % lower than the strength of the “pure” 3Y-TZP or 5Y-TZP zirconia layers; thus, Kaizer, for instance, is of the view that the clinical indication for Multilayer should not be expanded, but rather limited [5].

Due to their opacity, 1st Generation zirconias are mainly used as framework materials. It is possible to veneer them with feldspathic ceramics in order to obtain a natural looking tooth-colored restoration. The recurrent problems with chipping, especially in combination with implant restorations [10], can be reduced through standardized and optimized processing protocols [14]. It is important to note that, in contrast to metal ceramics, the processing

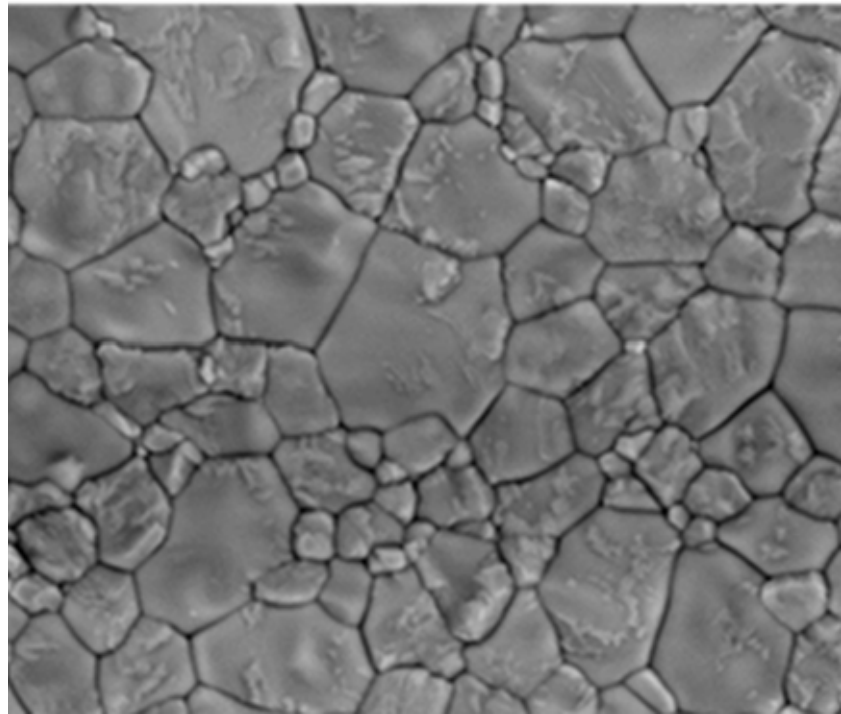


Figure 2 Scanning electron microscope imaging of the surface of 5Y-zirconia (magnification: 10,000x). Note the larger particle size compared to 3Y-zirconia (Fig. 1).

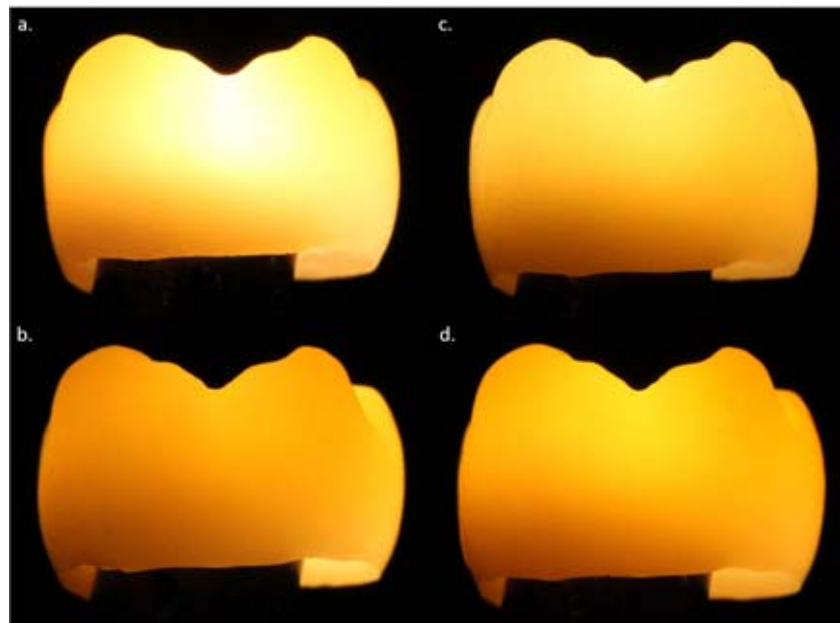


Figure 3a–d Illustration of the different translucency degrees of different ceramic materials. This example uses a molar crown for tooth 46. View from lingual using light guide illumination. All crowns were made of different materials (a–d), but with the aid of the same digital dataset using CAD/CAM, the crowns all have identical wall thicknesses. (a) Ivoclar emax CAD (Ivoclar-Vivadent, Schaan, FL); (b) Pritidenta multidisc ZrO₂ (Pritidenta, Leinfelden, D); (c) Ivoclar emax ZIRCAD Prime (upper position in Multilayer blank selected) (Ivoclar-Vivadent, Schaan, FL); (d) Ivoclar emax ZIRCAD Prime (lower position in Multilayer blank selected) (Ivoclar-Vivadent, Schaan, FL)

possibilities of zirconia are considerably smaller. For example, local temperature increases during the grinding of metal-ceramics is relatively well distributed by the metal lattice

structure, whereby the lattice structure of the ceramic leads to high temperature gradients. Due to the large temperature differences within closely spaced crystal structures, ini-

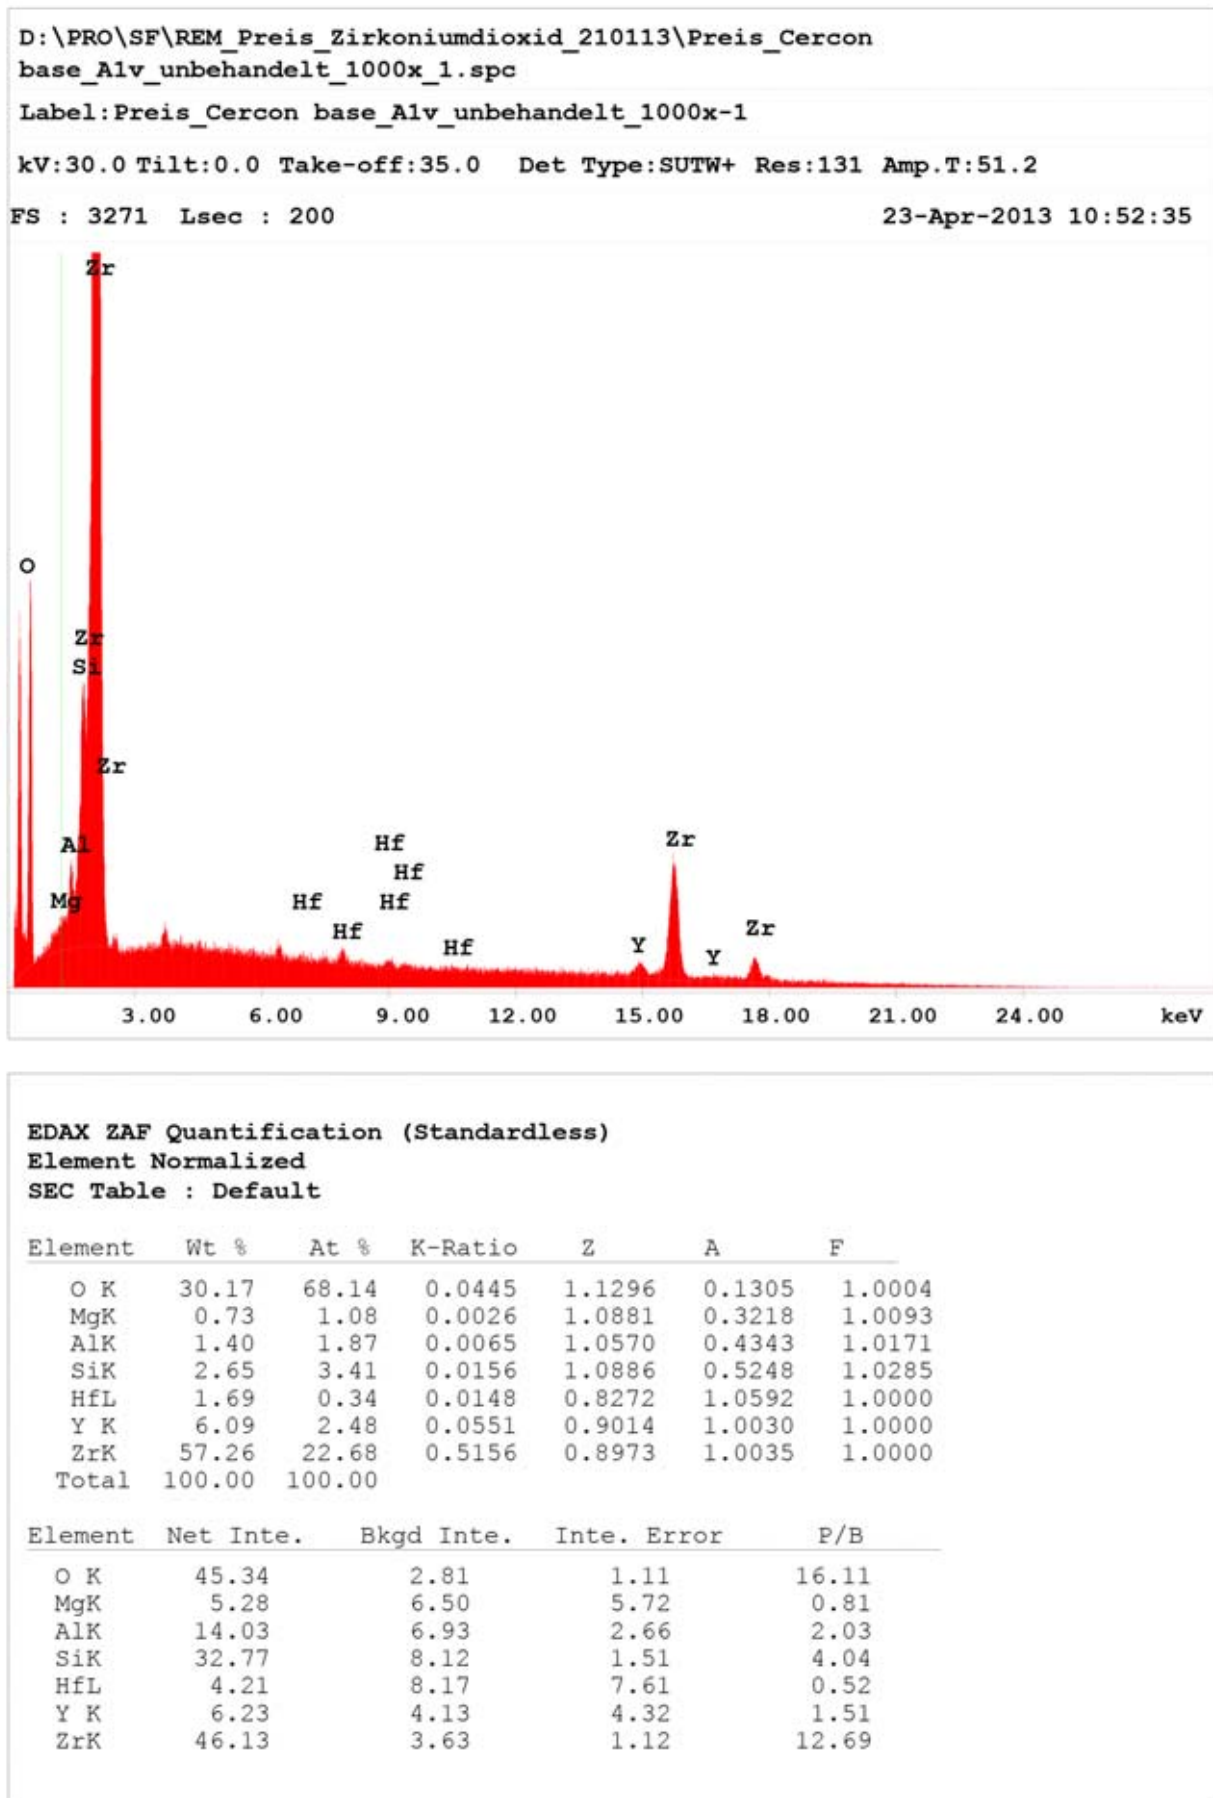


Figure 4 Plot of an EDX analysis (energy dispersive X-ray spectroscopy) of a 3Y-zirconia surface. The plot shows the chemical elements found in the sample: Zr, Al, Mg, Y, Hf, O, Si.

tial cracks form, which then propagate during the period of use, and can then contribute to premature failure, such as chipping.

Besides the clinical concerns regarding chipping, the new digital design possibilities for directly designing teeth with functional occlusal surfaces has also fuelled the desire to process esthetically appealing restorations with more translucent zirconia using a single class of materials by means of CAD/CAM. By doping zirconium dioxide with 5 mol-% yttrium oxide, abbreviated as “5Y-TZP”, this requirement is fulfilled and the translucency partially reaches that of lithium disilicate ceramics [13]. However, this advantage of increased translucency is offset by the disadvantage of reduced flexural strength, which reduces the clinical indication range of this type of zirconia. In fact, the indication range for 5Y-TZP zirconia hardly differs from that of lithium disilicate ceramics [14]. Apart from single crowns in the anterior and posterior areas, it only includes three-unit bridges in the anterior and premolar region. Bridges in molar area and the replacement of more than one pontic are usually not permitted. With 4th Generation zirconias (4Y-TZP), the strength is further increased so that a few manufacturers have expanded the indication range to include that of the molar region. In this case, in the planning phase of a restoration, the differing specifications from the manufacturers should already be taken into account.

What all zirconias have in common is that their wear pattern differs significantly from that of enamel or previous restorative materials [12, 15]; they practically do not wear. Due to this fact, if wear-resistant monolithic restorations are distributed unfavorably in the dentition, occlusal changes that affect the position of the masticatory plane may result. Thereafter, functional interferences cannot be ruled out [2]. In order to avoid damage to the antagonist teeth, it is essential to always perfectly polish monolithic zirconia to a high gloss following occlusal corrections [8, 11]. If this measure is omitted, antagonist teeth will become disproportionately damaged through abrasion [12].

Moreover, the safety of zirconia as a material in clinical applications requires attention because the starting material for clinically used zirconia is the mineral “zircon”, which is a carrier of natural radioactivity [1, 16]. Besides zirconium silicate, it contains hafnium oxide, thorium oxide and uranium oxide. These “impurities” must be removed from the material and this is achieved for thorium oxide and uranium oxide. The small traces of hafnium (Fig. 4), which usually remain detectable in zirconium dioxide, are nevertheless harmless. However, an unsatisfactory fact is that the Medical Devices Act [9] does not contain any regulations regarding the purity of zirconium dioxide used for medical purposes as of yet and that its treatment processes are not very transparent. Problems with hip joint prostheses from the 1990s show [3] that vigilance is required in this aspect.

Conclusion

Depending on their yttrium/aluminum doping ratio, dental zirconias show different properties. Zirconias with higher translucency have reduced mechanical strength compared to classical opaque zirconias. Due to this fact, their clinical indication range is limited. In fact, the clinical indications for translucent zirconias hardly differ from those of lithium disilicates. The restriction or broadening of the indication range to include the molar region must be carefully considered on a case-by-case basis in relation to the manufacturer, especially with respect to 4Y-TZP zirconias. Particularly confusing is the widely varying indication range for the new 5th Generation mixed zirconias with graded translucency within a milling block. For this generation, the indication range varies from only small three-span bridges in the anterior region [6] up to the approval of 14-unit bridges [4] (maximum of 2 teeth per dental gap replaced). Therefore, nowadays, the concept of “the zirconia” does not exist, but rather a multitude of material variants, which are created for individualized applications.

Michael Behr, Julian Füllerer,
Thomas Strasser, Verena Preis,
Julian Zacher, Regensburg

References

- Behr M: Dentales Zirkonium und Strahlenexposition. In: Staehle HJ (Hrsg): Deutscher Zahnärzte Kalender 2015, Deutscher Ärzteverlag, Köln 2015, 11–16
- Behr M, Proff P, Rosentritt M: Führt die Anwendung von monolithischem Zirkoniumdioxid möglicherweise zu Funktionsstörungen? Dtsch Zahnärztl Z 2019; 74: 86–89
- Cale B, Peille CN: Radioactive properties of ceramic hip joint heads. In: Heimke G (Hrsg): Bioceramic 1990, 152–159
- Ivoclar Vivadent: IPS e-max ZirCAD Prime Gebrauchsanweisung. <https://www.ivoclarvivadent.com/de/p/alle/produkte/vollkeramik/ips-emax-techniker/ips-emax-zircad>, (last access: 02.01.2020)
- Kaizer MR, Kolakarnprasert N, Rodrigues C, Chai H, Zhang Y: Probing the interfacial strength of novel multi-layer zirconias. Dent Mater 2020; 36: 60–67
- Kuraray Noritake Europe: Gebrauchsanleitung Katana Keramik UT (Ultra Translucent) & UTML (Ultra Translucent Multi Layered), Hattersheim 2017
- Lohbauer U, Belli R, Wendler M: Keramische Materialien. In: Rosentritt M, Ilie N, Lohbauer U (Hrsg): Werkstoffkunde in der Zahnmedizin. Moderne Materialien und Technologien. Thieme, Stuttgart, New York 2018, 239–305
- Matzinger M, Hahnel S, Preis V, Rosentritt M: Polishing effects and wear performance of chairside CAD/CAM materials. Clin Oral Investig 2019; 23: 725–737
- Medizinproduktegesetz in der Fassung der Bekanntmachung vom 7. August 2002 (BGBl. I S. 3146), das zuletzt durch Artikel 83 des Gesetzes vom 20. November 2019 (BGBl. I S. 1626) geändert worden ist“ 2019
- Pjetursson BE, Valente NA, Stranding M, Zwahlen M, Liu S, Sailer I: A systematic review of the survival and complication rates of zirconia-ceramic and metal-ceramic single crowns. Clin Oral Implants Res 2018; 29(Suppl 16): 199–214
- Preis V, Grumser K, Schneider-Feyrer S, Behr M, Rosentritt M: The effectiveness of polishing kits. Influence on surface roughness of zirconia. Int J Prosthodont 2015; 28: 149–151
- Preis V, Grumser K, Schneider-Feyrer S, Behr M, Rosentritt M: Cycle-dependent in vitro wear performance of dental ceramics after clinical surface treatments. J Mech Behav Biomed Mater 2016; 53: 49–58
- Rosentritt M, Kieschnick A, Stawarczyk B: Zahnfarbene Werkstoffe im

Vergleich. Kleine Werkstoffkunde für Zahnärzte – Teil 4. ZM-online 2019

14. Rosentritt M, Kiesneck A, Hahnel S, Stawarczyk B: Werkstoffkunde-Kompendium Zirkonoxid. Moderne dentale Materialien im Arbeitsalltag. <https://werkstoffkunde-kompendium.de/das-werkstoffkunde-kompendium/zirkonoxid/>, (last access: 27.01.2020)

15. Rosentritt M, Schumann F, Krifka S, Preis V: Influence of zirconia and lithium disilicate tooth- or implant-supported crowns on wear of antagonistic and adjacent teeth. *J Adv Prosthodont* 2020; 12: 1–8

16. Rösler HL: Lehrbuch der Mineralogie. Deutscher Verlag für Grundstoffindustrie, Leipzig 1991



(Photo: UKR)

PROF. DR. MED. DENT.
MICHAEL BEHR
University of Regensburg
Faculty of Medicine
Franz-Josef-Strauss-Allee 11
93053 Regensburg
michael.behr@klinik.uni-regensburg.de